

**Operating Instructions
for
Pressure Sensors**

Model: SEN-3



1. Contents

1. Contents.....	2
2. Note	3
2.1. Notes on the machine and pressure equipment directive	3
3. Regulation Use	3
4. Operating Principle.....	4
5. Instrument Inspection.....	4
6. Mechanical Connection.....	5
7. Electrical Connection	6
8. Trouble Shooting.....	8
9. Maintenance	9
10. Technical Information.....	9
11. Order Codes	9
12. Dimensions	9
13. Disposal	10
14. EU Declaration of Conformance	11
15. UK Declaration of Conformity.....	12

Manufactured and sold by:

Kobold Messring GmbH
Nordring 22-24
D-65719 Hofheim
Tel.: +49(0)6192-2990
Fax: +49(0)6192-23398
E-Mail: info.de@kobold.com
Internet: www.kobold.com

2. Note

Please read these operating instructions before unpacking and putting the unit into operation. Follow the instructions precisely as described herein.

The instruction manuals on our website www.kobold.com are always for currently manufactured version of our products. Due to technical changes, the instruction manuals available online may not always correspond to the product version you have purchased. If you need an instruction manual that corresponds to the purchased product version, you can request it from us free of charge by email (info.de@kobold.com) in PDF format, specifying the relevant invoice number and serial number. If you wish, the operating instructions can also be sent to you by post in paper form against an applicable postage fee.

The devices are only to be used, maintained and serviced by persons familiar with these operating instructions and in accordance with local regulations applying to Health & Safety and prevention of accidents.

2.1. Notes on the machine and pressure equipment directive

When used in machines, the measuring unit should be used only when the machines fulfil the EC-machine guidelines.

as per PED 2014/68/EU

"Pressure gauges with a volume ≤ 0.1 L"

In acc. with Article 4 Paragraph (3), "Sound Engineering Practice", of the PED 2014/68/EU no CE mark.

Diagram 2

Vessels referred to in Article 4(1)(a)(i), second indent

3. Regulation Use

Any use of the Pressure Sensors Model: SEN-3 which exceeds the manufacturer's specification may invalidate its warranty. Therefore, any resulting damage is not the responsibility of the manufacturer. The user assumes all risk for such usage.

4. Operating Principle

Pressure sensors transmit the mechanical quantity pressure into an electrical output signal. The media's which are in contact with the instrument should be chemically compatible with the instrument materials used. Do not use standard sensors in hazardous areas and for oxygen applications.

5. Instrument Inspection

Instruments are inspected before shipping and sent out in perfect condition. Should the damage to a device be visible, we recommend a thorough inspection of the delivery packing. In case of damage, please inform your parcel service / forwarding agent immediately, since they are responsible for damages during transit.

Scope of delivery:

- Pressure Sensors model: SEN-3


6. Mechanical Connection

The places where pressures are taken should be prepared according the following specifications for the screw-in threads. This is very important for pressure sensors with front diaphragm, because otherwise the diaphragm could be damaged. For sealing, please use sealing discs acc. DIN 16258 or profile washers. The maximum initial tension depends on the material, the shape of the used sealing and the mechanical connection of the pressure sensor. The given tensions should not be exceeded.


- 50 Nm for pressure sensors with metallic sealing cone (hereby, there could be for small measure ranges a deviation of the zeropoint of maximum 1%. This deviation could be adjusted, with the zero point potentiometer see chapter "Maintenance").
- 80 Nm for pressure sensors with pressure connection acc. DIN 16288, and/or flash front diaphragm with O-ring.

There should be no vibrations and/or no radiation of heat near the mounting position of the sensors. Please pay attention that the giving operating limits are not exceeded. After the mechanical and electrical connection, the sensor is ready for operation.


Screw in hole for diaphragm on inside





Sealing acc. DIN 16288

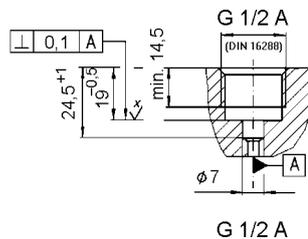


Sealing with flat gasket ring



Screw in hole/Screw in socket for flush front diaphragm with o-ring sealing



with metalical sealing cone

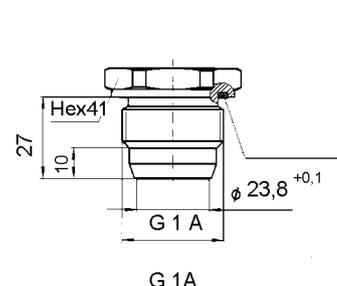

7. Electrical Connection

- Ensure that the power is disconnected during connection of the cable.
- The electrical connection is made either via plug and pin or by cable.
- The exact wiring scheme is shown on the sketches hereafter or at the type plate of your sensor.

Attention! to the different wire systems.

Meaning of the different connector markings

UB+	positive pole of the supply voltage
OV	negative pole of the supply voltage
S+	positive pole of the output signal
S-	negative pole of the output signal
Shielding	Cable protection enclosure-earth

Pressure sensors for relative pressures with cable output are equipped with an atmospheric pressure compensation cable. Please take this into account if you want to extend the cable. The relative pressure sensor with pressure ranges up to 25 bar are vented due to a venting sealing between housing and plug. The sensor could be supplied with an unregulated DC source with the specified voltage range. The minimum supply voltage for pressure sensors with current output, should be the minimum UB plus the minimum voltage, which is needed to operate the external indicator or input device:

Current output

	2-wire system	3-wire system
Output signal	4...20 mA	0...20 mA
Supply voltage	$U_B = 10 \dots 30 V_{DC}$	
Permissible load	$RA[Ohm] = (U_B[V] - 10 V) / 0,02 A$	
Wiring scheme	see scheme	

Voltage output


	3-wire system	3-wire system
Output signal	0...5 V	0...10 V
Supply voltage	$U_B = 10 \dots 30 V_{DC}$	$U_B = 14 \dots 30 V_{DC}$
Permissible load	$RA > 5 kOhm$	$RA > 10 kOhm$
Wiring scheme	see scheme	

Electrical connection, principle drawings, pin assignment, cable marking


2-wire-system

DIN 43650 plug


5-pin M12 connector

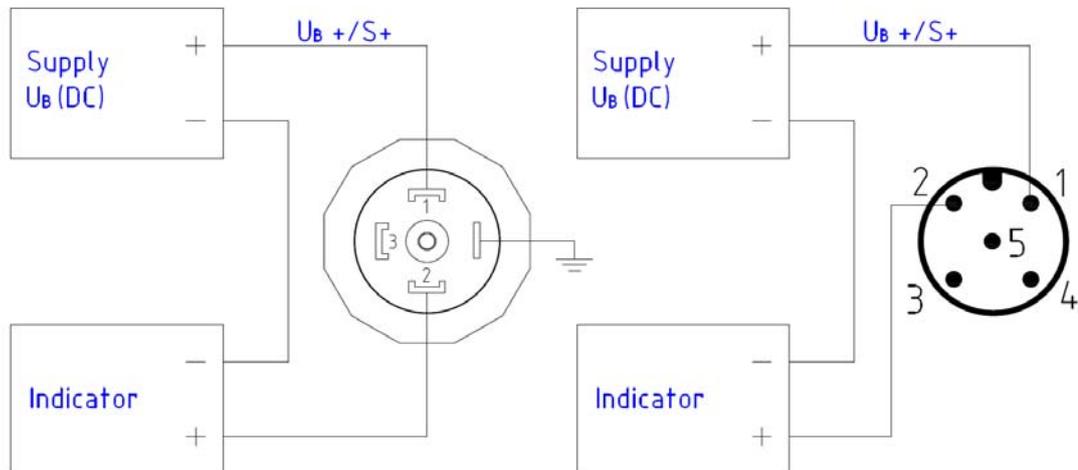

3-wire-system

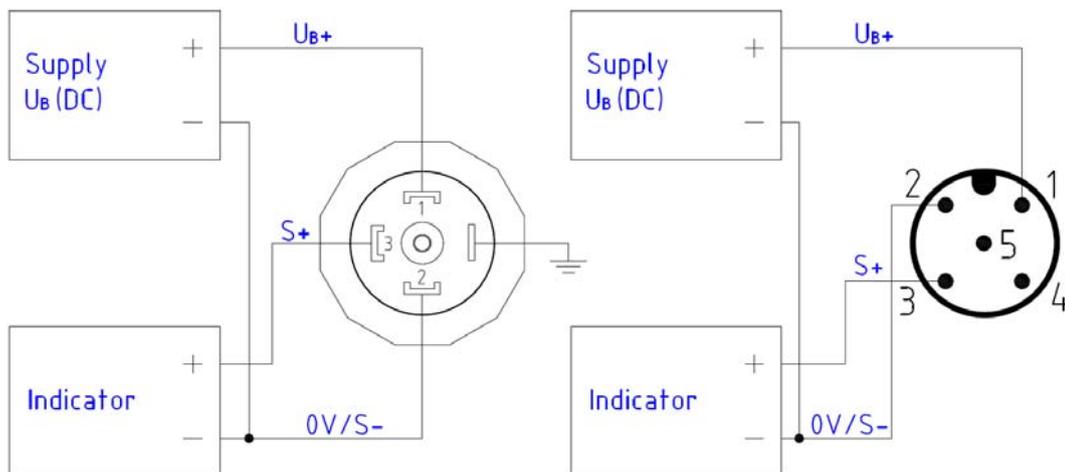

free cable

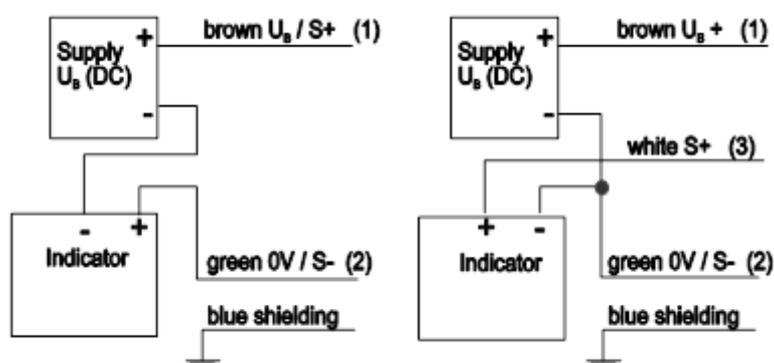

8. Trouble Shooting

Trouble	Possible reason	What's to do
No signal	no supply voltage broken wire	Check your power supply and wiring. If necessary replace defective parts
	Sensor has been wired improperly	Check the wiring according to the sketches and adjust wiring if necessary.
	No pressure	Check your tubing, valves open?
	Defective electronics caused by excessive supply voltage or by external voltage	Return sensor to us for repair
Unchanged signal by changing pressure	Pressure port is blocked	Clean the pressure port
	Defective electronics caused by excessive supply voltage or by external voltage	Return sensor to us for repair
	Pressure sensor over pressurized	Return sensor to us for repair
To high, even on changing pressure unchanged signal	Defective electronics caused by excessive supply voltage or by external voltage	Return sensor to us for repair
Span of signal too small	Supply voltage too low or loop resistance too high	Adjust supply voltage to overcome loop resistance
	Span adjustment potentiometer deregulated	Recalibrate sensor
Zero Signal too low	Zero adjustment potentiometer deregulated	Recalibrate sensor
Zero signal too high	Zero adjustment potentiometer deregulated	Recalibrate sensor
	Mechanical damage	Recalibrate sensor Return to us for repair
Output signal non linear	Mechanical damage	Recalibrate sensor Return to us for repair

9. Maintenance

The pressure sensors described in this manual are maintenance free! They do not contain any components which may be repaired or exchanged locally. Repairs are only possible in our factory.

10. Technical Information

Operating instructions, data sheet, approvals and further information via the QR code on the device or via www.kobold.com

11. Order Codes

Operating instructions, data sheet, approvals and further information via the QR code on the device or via www.kobold.com

12. Dimensions

Operating instructions, data sheet, approvals and further information via the QR code on the device or via www.kobold.com


13. Disposal

Note!

- Avoid environmental damage caused by media-contaminated parts
- Dispose of the device and packaging in an environmentally friendly manner
- Comply with applicable national and international disposal regulations and environmental regulations.

Batteries

Batteries containing pollutants are marked with a sign consisting of a crossed-out garbage can and the chemical symbol (Cd, Hg, Li or Pb) of the heavy metal that is decisive for the classification as containing pollutants:

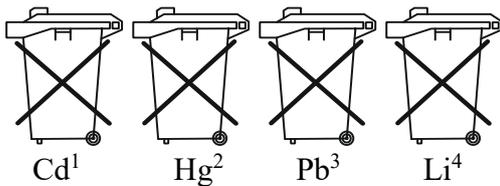

1. „Cd" stands for cadmium
2. „Hg" stands for mercury
3. „Pb" stands for lead
4. „Li" stands for lithium

Electrical and electronic equipment



14. EU Declaration of Conformance

We, KOBOLD Messring GmbH, Nordring 22-24, 65719 Hofheim, Germany, declare under our sole responsibility that the product:

Pressure Sensor Model: SEN-3...

to which this declaration relates is in conformity with the following EU directives stated below:

2014/30/EU	EMC Directive
2011/65/EU	RoHS (category 9)

Also, the following standards are fulfilled:

EN 61326-1:2013

Electrical equipment for measurement, control and laboratory use - EMC requirements - Part 1: General requirements

EN 61326-2-3:2013

Electrical equipment for measurement, control and laboratory use - EMC requirements - Part 2-3: Particular requirements - Test configuration, operational conditions and performance criteria for transducers with integrated or remote signal conditioning

EN IEC 63000:2018 Technische Dokumentation zur Beurteilung von Elektro- und Elektronikgeräten hinsichtlich der Beschränkung gefährlicher Stoffe

Hofheim, 10. October 2023



H. Volz
General Manager

J. Burke
Compliance Manager

15. UK Declaration of Conformity

We, KOBOLD Messring GmbH, Nordring 22-24, 65719 Hofheim, Germany, declare under our sole responsibility that the product:

Pressure Sensor Model: SEN-3...

to which this declaration relates is in conformity with the following UK directives stated below:

S.I. 2016/1101 Electrical Equipment (Safety) Regulations 2016
S.I. 2012/3032 The Restriction of the Use of Certain Hazardous
Substances in Electrical and Electronic Equipment Regulations 2012

Also, the following standards are fulfilled:

BS EN 61326-1:2013

Electrical equipment for measurement, control and laboratory use. EMC requirements. General requirements

BS EN 61326-2-3:2013

Electrical equipment for measurement, control and laboratory use. EMC requirements. Particular requirements. Test configuration, operational conditions and performance criteria for transducers with integrated or remote signal conditioning

BS EN IEC 63000:2018

Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances.

Hofheim, 10. October 2023



H. Volz
General Manager

J. Burke
Compliance Manager